




Jada

The Jada® System is intended to provide control and treatment of abnormal postpartum uterine bleeding or hemorrhage when conservative management is warranted.¹

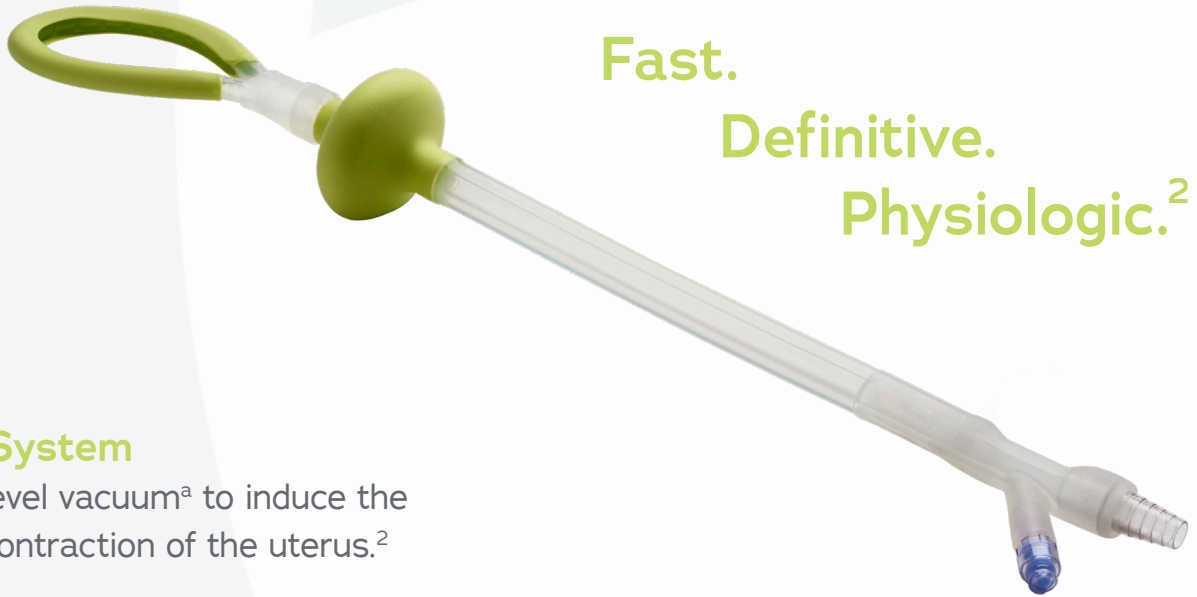

**Fast.
Definitive.
Physiologic.²**


The Jada System

utilizes low-level vacuum^a to induce the physiologic contraction of the uterus.²




94% Effectiveness

94% (n=100/106) of participants treated successfully in the PEARLE study with the Jada System ($P < 0.001$).^{2,b}

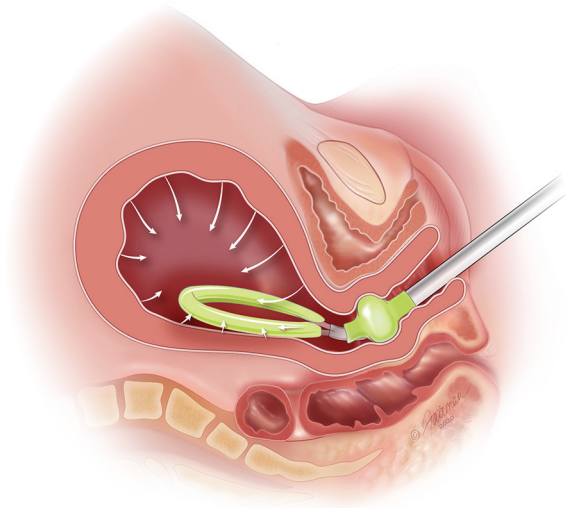

Low-level vacuum^a induces collapse of the atonic postpartum uterus²

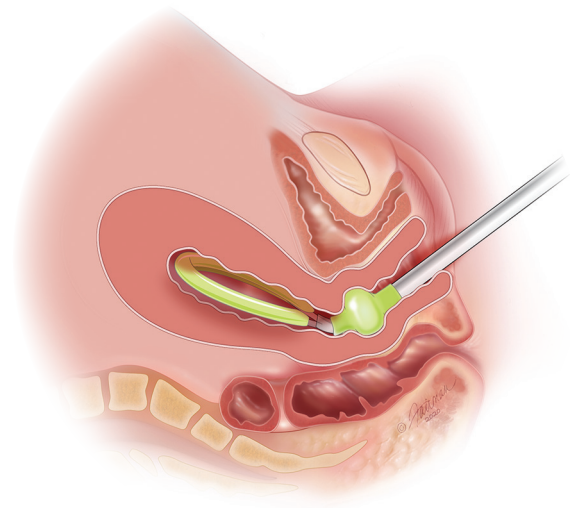

Contraction of the myometrium provides physiologic control of bleeding²

^a80 mm Hg +/- 10 mm Hg. The maximum vacuum pressure is 90 mm Hg. Do not increase the vacuum pressure higher than 90 mm Hg or tissue trauma may occur.¹

^bPrimary effectiveness was the control of postpartum hemorrhage, defined as the avoidance of non-surgical, second line or surgical intervention to control uterine hemorrhage.²




The PEARLE study was a prospective, single-arm, literature-controlled, multi-center treatment study of 107 subjects (comparator was a meta-analysis of the Bakri® Postpartum Balloon). The study was designed to assess the safety and effectiveness of the Jada System in treating primary postpartum hemorrhage & abnormal postpartum uterine bleeding.^{2,3}

Fast



Bleeding can be controlled within minutes.²

Minutes
(median)

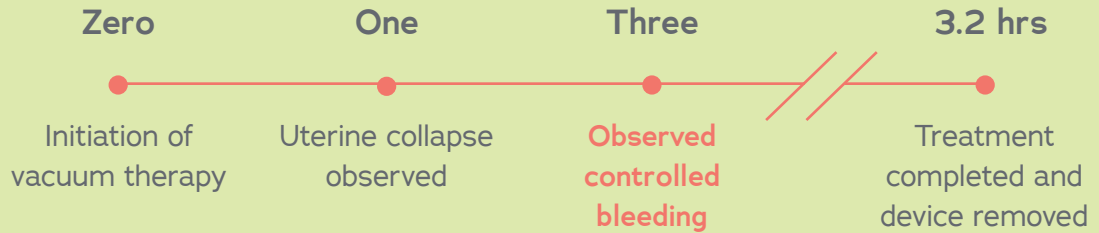


Definitive

Visible and observable control of hemorrhage and bleeding²

Physiologic

Vacuum induces a physiologic contraction of the uterus to control and treat the abnormal postpartum uterine bleeding and hemorrhage^{2,a}

Highly rated by investigators^{2,3}



Would recommend Jada
n=104/107



Reported Jada was easy to use
n=105/107

Favorable safety profile³

There were no adverse events judged definitely related to the device or the procedure and there was a low rate of possibly related adverse events.

- 5 possibly device-related adverse events were rated as “moderate” and no event was rated as “severe.”
- 3 moderate events were cases of endometritis, which is a known risk of long labor, vaginal exam, and PPH.

Please refer to the Jada System Instructions for Use for indications, contraindications, warnings, precautions, and other information at [thejadasystem.com/ifu](https://www.thejadasystem.com/ifu)

References: 1. Jada System. Vacuum-induced Hemorrhage Control System: Instructions for Use. Alydia Health; 2020. 2. D'Alton ME, Rood KM, Smid MC, et al. Intrauterine vacuum-induced hemorrhage-control device for rapid treatment of postpartum hemorrhage. *Obstet Gynecol.* 2020;136(5):882-891. doi:10.1097/AOG.0000000000004138 3. Data available on request from Professional Services-DAP (Marketing Operations), 1180 Church Road, Lansdale, PA 19446. Please specify information package US-JDA-110046.